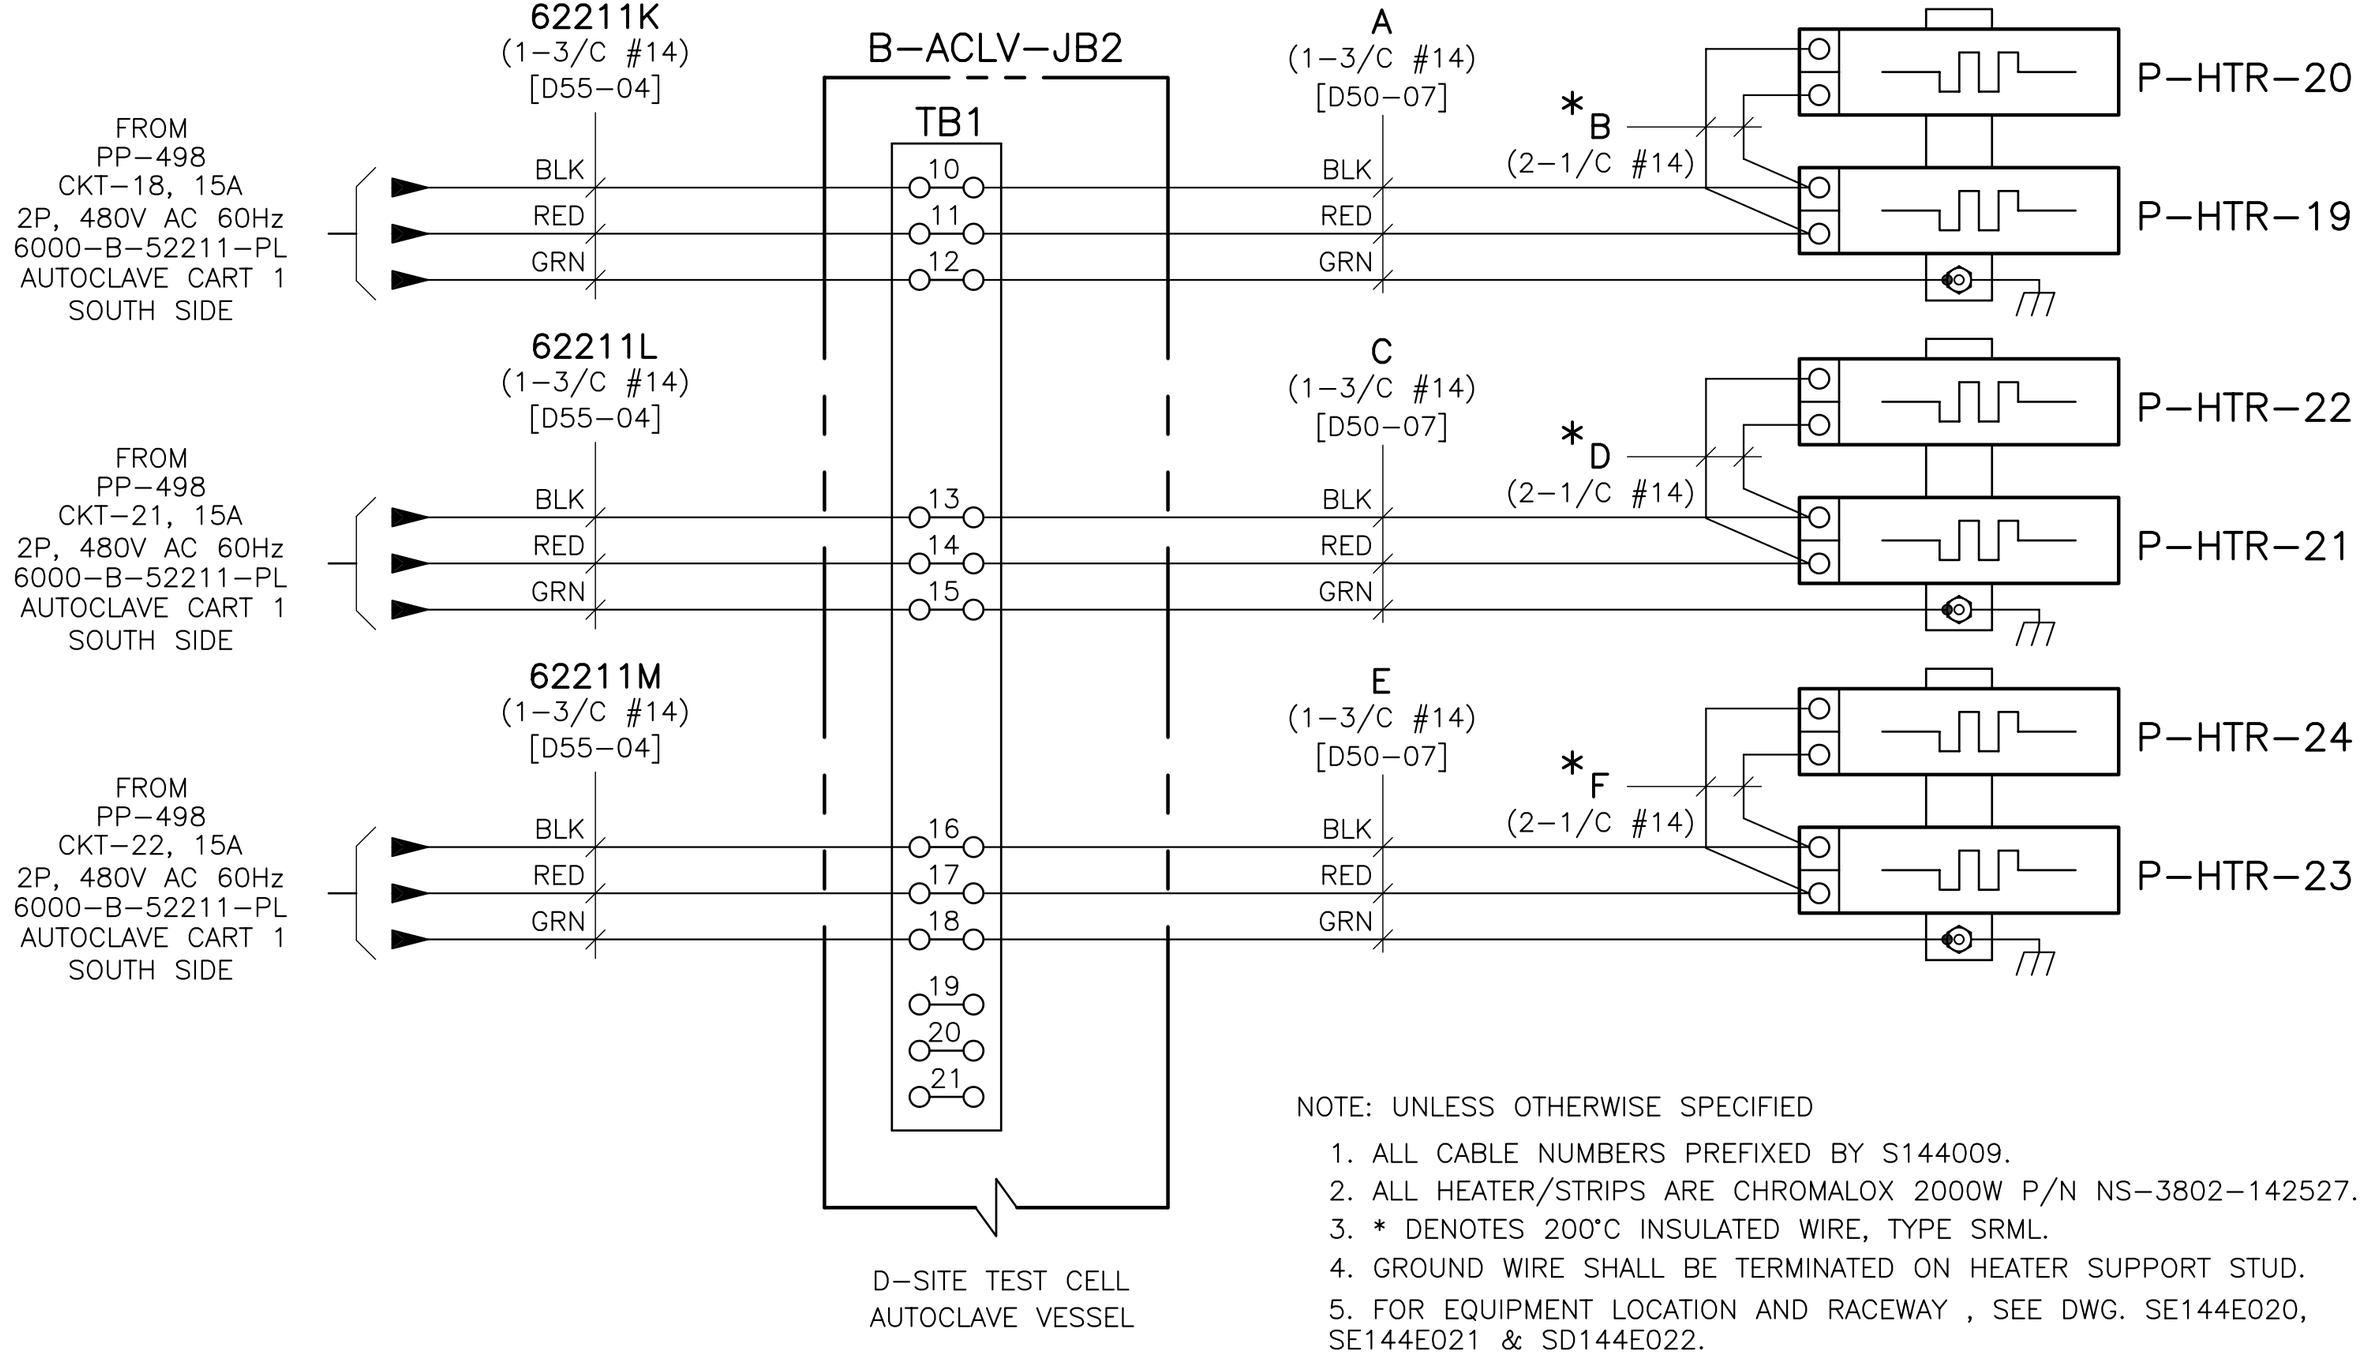


NOTE: UNLESS OTHERWISE SPECIFIED

1. ALL CABLE NUMBERS PREFIXED BY S144009.
2. ALL HEATER/STRIPS ARE CHROMALOX 2000W P/N NS–3802–142527.
3. * DENOTES 200°C INSULATED WIRE, TYPE SRML.
4. GROUND WIRE SHALL BE TERMINATED ON HEATER SUPPORT STUD.
5. FOR EQUIPMENT LOCATION AND RACEWAY , SEE DWG. SE144E020, SE144E021 & SD144E022.

COMPUTER GENERATED DRAWING – MANUAL CHANGES NOT PERMITTED

CADD FILE NUMBER SB144E009.DWG

| REV | DATE | BY | APPROVED | REV | DATE | BY | APPROVED |
|---|---|---|---|---|---|---|---|
| 8 | | | | 4 | | | |
| 7 | | | | 3 | | | |
| 6 | | | | 2 | | | |
| 5 | | | | 1 | | | |

DIV ELECTRICAL
ENG F.JONES
DR RVK CH JJN
DATE 2–07–03

APPROVED
F. JONES
DATE 2/03

| CH | SUPV |
|---|---|
| JJN | JS |

PLASMA PHYSICS LABORATORY
PRINCETON UNIVERSITY
NATIONAL COMPACT STELLARATOR EXPERIMENT
MODULAR COILS
TOOLING AND WINDING
AUTOCLAVE 2000W PRIMARY HTR 19–24

NCSX
SB144E009
SH 1