

Princeton Plasma Physics Laboratory Procedure

Procedure Title: **Field Period Assembly Station One**

Number:
D-NCSX-FPA-001

Revision:
0

Effective Date: **June 15, 2006**

Expiration Date:
(2 yrs. unless otherwise stipulated)

Procedure Approvals

Author: John W. Edwards:

ATI: Mike Viola:

RLM: Larry Dudek:

Responsible Division: **NCSX Project**

Procedure Requirements Designated by RLM

LABWIDE:

X	Work Planning Form (ENG-032) #1224		Lockout/Tagout (ESH-016)
	Confined Space Permit (5008,SEC.8 Chap 5)		Lift Procedure (ENG-021)
	Master Equip. List Mod (GEN-005)	X	ES&H Review (NEPA, IH, etc.) NEPA 1283
	RWP (HP-OP-20)		Independent Review
	ATI Walkdown	X	Pre-Job Brief
X	Post-job Brief *	X	Hydrostatic and Pneumatic Testing. (ENG-014)

D-SITE SPECIFIC:

X	D-Site Work Permit (OP-AD-09)		Door Permit (OP-G-93)
	Tritium Work Permit (OP-AD-49)		USQD (OP-AD-63)
X	Pre-Job Brief (OP-AD-79)		T-Mod (OP-AD-03)
	** DCA/DCN (OP-AD-104) #		

- * Required for installations involving internal vacuum installations, critical lifts, and for the initial installation of repetitive work.
- ** OP-AD-104 was voided by procedure ENG-032. However, DCA's that were open at the time of adoption of ENG-032 are still considered valid for work approval purposes.

REVIEWERS (designated by RLM)		Rec'd/ Incorp. Comments
Accountable Technical Individual. John W Edwards		
Test Director		
Independent Reviewer		
D-Site Shift Supervisor		
Independent		
NCSX Dimensional Control Coordinator Brent Stratton		
Vacuum Vessel Cognizant Engineer..... Paul Goranson		
NCSX Field Supervisors... Steve Raftopoulos, Mike Viola		X
Project Engineer for Stellerator Systems (WBS 1) Manager..... Brad Nelson (ORNL)		
FPA Tooling and Constructability..... Tom Brown		X
Quality Assurance/Quality Control. Frank Malinowski		X
Maintenance and Operations Division		
Energy Conversion System/Motor Control Division		
Engineering Wayne Reiersen		
Environmental Restoration & Waste Management Division		
Environmental, Safety & Health..... Jerry Levine		X
Industrial Hygiene..... Bill Slavin		
Health Physics..... George Ascione		
RLM Larry Dudek		X

TRAINING (designated by RLM)			
No training required _____		Instructor John Edwards	
Personnel (group, job title or individual name)	Read Only	Instruction Pre-job Briefing	Hands On
Lead Tech.		X	
Technicians performing task		X	
Field Supervisors		X	
Quality Control Representative		X	
Training Rep.			
RLM Larry Dudek			

**Field Period Assembly Station One
D-NCSX-FPA-001**

RECORD OF CHANGE

Revision	Date	Description of Change
00	XXXX	Initial release

TABLE OF CONTENTS

1. Scope.....	1
1.1. Introduction.....	1
1.2. Scope.....	1
1.3. Identification of Vacuum Vessel Segment:.....	1
2. Applicable Documents.....	1
2.1. NCSX-MIT/QA-185-00:.....	1
2.2. NCSX-PLAN-CMFOP-00:.....	1
2.3. D-L-NCSX-997 Lifting Vacuum Vessel Segment.....	1
2.4. D-NCSX-PLAN-FPA1DC-00 VV Dimensional Control Plan.....	1
3. Safety Requirements:.....	1
3.1. Job Hazard Analysis:.....	1
4. Prerequisites & Conditions:.....	2
4.1. Pre-Job Briefing:.....	2
4.2. Daily Operations Startup and Shutdown:.....	2
5. Materials and Parts for this station.....	2
6. Assembly Process.....	2
6.1. Daily Startup Activities:.....	3
6.2. Daily Shutdown Activities:.....	3
6.3. Vacuum Vessel Receipt Inspection.....	3
6.4. Replace Port Flanges with Station 1 Assembly Flanges:.....	4
6.5. Cg verification and Install VV in Station One Rotating Fixture.....	5
6.6. Metrology Set-Up and Initial Vessel Measurements:.....	7
6.7. Marking Flux Loop Template and Heating Coolant Stud Locations:.....	8
6.8. Vertical Port Component Installation:.....	9
6.9. Installation of Magnetic Flux Loop Templates:.....	10
6.10. Installation of Magnetic Flux Loops:.....	11
6.11. H/C Stud and Loop Wires Installation:.....	12
6.12. Final Loop Routing and Measurement:.....	13
6.13. H/C line Installation:.....	13
6.14. Loop Termination and Verification Check:.....	14
6.15.
6.16.
6.17.
6.18.
6.19.
6.20.

**Field Period Assembly Station One
D-NCSX-FPA-001**

6.21.	
6.22.	
6.23.	
7.	Completion of Activities at Station One:	15
7.1.	Document Verification:	15
7.2.	Field Package:	15
7.3.	Approval:	15
7.4.	Preparing and Transferring Completed VV to Station 3:	15
8.	Appendix A Document Sign Off Record:	17

Index of Figures

Figure 1-	Horizontal Flange.....	3
Figure 2-	Heating and Cooling Cryostat Interface Flanges.....	4
Figure 3-	Vacuum Vessel in Horizontal Position	4
Figure 4-	Worm Drive Installation Details.....	5
Figure 5-	Toroidal Field Direction	6
Figure 6-	60° Off Vertical Position	6
Figure 7-	Vacuum Vessel in Rotated Position	7
Figure 8-	Templates Locating and Numbering.....	8
Figure 9-	Overlay of the Coolant Lines Over the Diagnostic Loops	9
Figure 10-	Cryostat Interface	9
Figure 11-	Heating strip	10
Figure 12-	Installing Loop Templates.....	11
Figure 13-	H/C Support Brackets.....	13
Figure 14-	Hard Tube Installation	14
Figure 15-	Angle Support Bracket and Base Support Plate	16
Figure 16-	Stage 3 Support Stand.....	16
Figure 17-	
Figure 18-	
Figure 19-	
Figure 20-	

Index of Tables

Table 1-	Loop Installation Data For Field Period #1:	20-22
Table 2-	Loop Installation Data For Field Period #2:	23-25
Table 3-	Loop Installation Data For Field Period #3:	26-28
Table 4-	Stud Installation Data For Field Period #1:.....	29
Table 5-	Stud Installation Data For Field Period #2:.....	30
Table 6-	Stud Installation Data For Field Period #3:.....	31
Table 7-	H/C/ Lines Installation and Leak Check Data For Field Period #1:.....	32
Table 8-	H/C/ Lines Installation and Leak Check Data For Field Period #2:.....	33
Table 9-	H/C/ Lines Installation and Leak Check Data For Field Period #3:.....	34

Field Period Assembly Station One

D-NCSX-FPA-001

1. Scope

1.1 Introduction

The Field Period Assembly is divided into 5 workstations. Each workstation has a specific set of tasks that will be performed as part of the overall assembly process. This procedure addresses the manufacturing, inspection, test and QC inspection points for a specific workstation.

- Station No. 1...Vacuum Vessel Subassembly (VVSA) Activities

1.2 Scope

This procedure is used to describe the assembly sequence required for Station 1 Field Period Assembly.

Installing the Vacuum Vessel in the turning fixture
Metrology measurements
Flux Loop Locations
Heating Cooling Tube Stud Location
Installation of Flux Loops
Installation of Heating –Cooling Tubes

1.3 Identification of Vacuum Vessel Segment being assembled:

See Appendix A – Document Sign-off-Record

2. Applicable Documents:

2.1 NCSX-MIT/QA-185-00:

All applicable documents associated with this procedure, are identified in the MIT/QA Plan, document number **NCSX-MIT/QA-185-00**.

2.2 NCSX-PLAN-CMFOP-00:

All work processes are governed by the “NCSX Coil Manufacturing Facility Operations Plan”, document number **NCSX-PLAN-CMFOP-00**.

2.3 D-L-NCSX-007 Lifting Vacuum Vessel Segment

2.4 D-NCSX-PLAN-FPA1DC-00 VV Dimensional Control Plan

3. Safety Requirements:

All work will be performed in a safe manner in accordance with PPPL Environmental Safety & Health Directives **ES&H 5008** and the “Integrated Safety Management” (ISM) policy.

3.1 Job Hazard Analysis:

A JHA will be generated for each Vacuum Vessel Sub Assembly station, identifying existing or potential workplace hazards and to evaluate the risk of worker injury or illness associated with job tasks. (Reference document **ESH-004 “Job Hazard Analysis”**) The IH representative will review the JHAs for accuracy as well as completeness. It will be reviewed with all activity participants at the Pre-Job briefings.

Field Period Assembly Station One D-NCSX-FPA-001

6.1 Daily Startup Activities:

- 6.1.1 Check all daily supplies needed:
- 6.1.2 Verify operation of all equipment needed that day.
- 6.1.3 Check station for cleanliness
- 6.1.4 Check that safety equipment needed for day's activities are available
- 6.1.5 Check that the day's travelers (I.E. Appendix A) and procedures are in their document holder.
- 6.1.5 Once completed, date and initial daily log at the back of the Station Log Book.

6.2 Daily Shutdown Activities:

- 6.2.1 Turn off power to equipment not in use.
- 6.2.2 Clean entire workstation area.
- 6.2.3 Verify that all Traveler (I.E. Appendix A) and data sheet information is complete.
- 6.2.4 The Lead Technician shall verify that the Station's Log Book has been completed and signed for the day.
- 6.2.5 Once completed, date and initial daily log at the back of the Station Log Book.

6.3 Replace Port Flanges with Station 1 Assembly Flanges:

- 6.3.1 If attached remove the two horizontal port flanges covers and bag bolt assemblies for future use. See Figure 1.

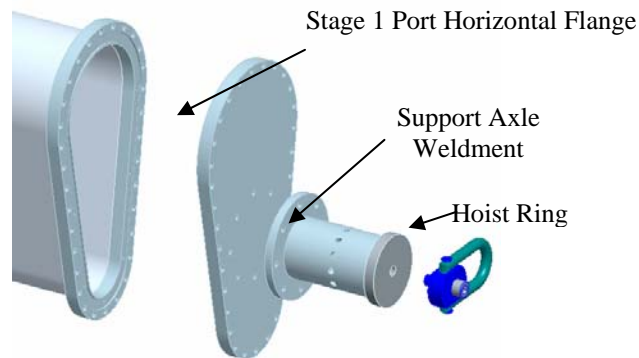


Figure 1. Horizontal Flange

- 6.3.2 If attached remove NB port flange and bag bolt assemblies for future use. Install temporary port cover se 184-054 and seal spacer se 184-055. See Figure 2.
- 6.3.3 Install VV heating/cooling cryostat interface flanges by slipping each over each vertical port. The interface flanges need to be temporarily supported on the flanges. Reference drawing: se123-164. See Figure 2

**Field Period Assembly Station One
D-NCSX-FPA-001**

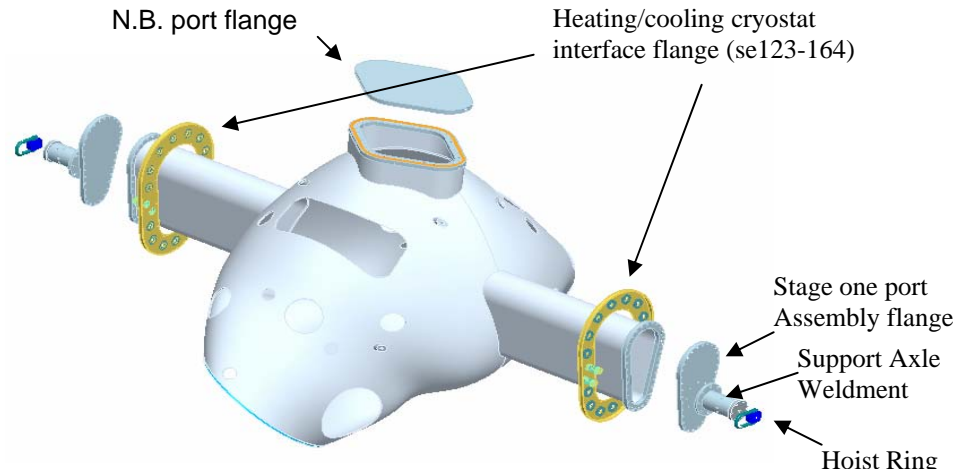


Figure 2 Heating and Cooling Cryostat Interface Flanges

6.3.6 Using rubber gasket material or gortex gasket material on the flanges for flange protection install stage one port assembly flange covers.

6.3.7 Using shim stock as needed to keep support axle weldments coaxial. Install support axle weldments to stage one port assembly flanges.

6.4 Install VVSA in Station One Rotating Fixture:

6.4.1 Using lift procedure (D-L-NCSX-997) and test cell crane, basket around the two VVSA port 12's. Lift VVSA enough to remove load from a base support then remove support base by grinding the welds off the support base to VVSA. Lift VVSA high enough too allow the VVSA base support to be removed from under the VVSA.

6.4.2 Lubricate support axle and axle support cradle. Add lubricant to support axle weldment and support axle cradle components (cradle top and cradle base) to reduce VV rotation friction.

6.4.3 Mount VV on Station one rotating fixture in the horizontal position. See Figure 3.

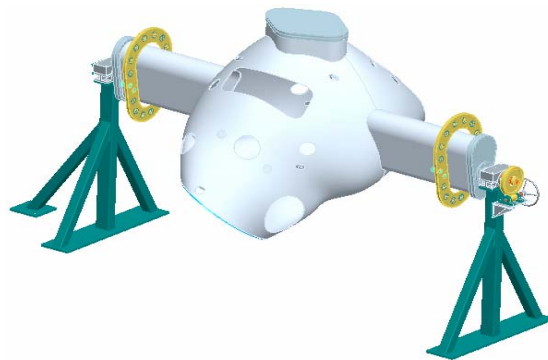


Figure 3 Vacuum Vessel in Horizontal Position

Field Period Assembly Station One D-NCSX-FPA-001

6.4.4 Secure in place by bolting down support axle cradle to support blocks. See Figure 4.

6.4.5 Install quick release pin. See Figure 4.

6.4.6 Install worm gear axle and worm gear. See Figure 4.

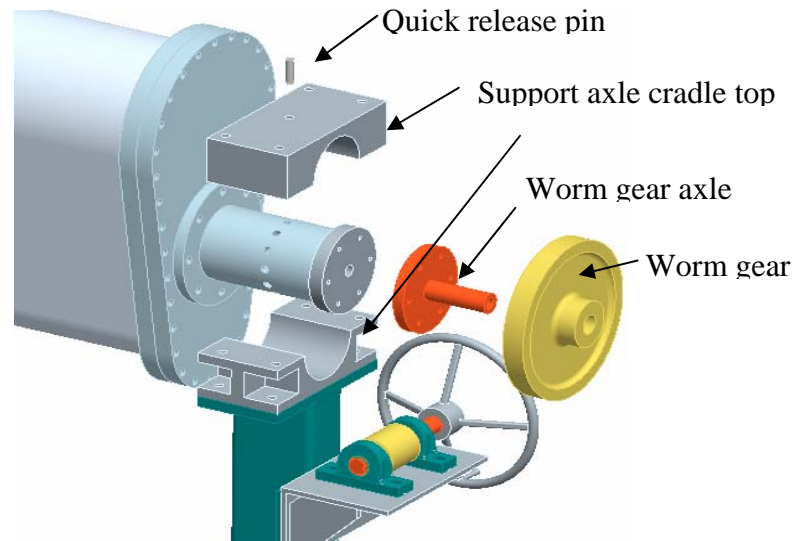


Figure 4 Worm Drive Installation Details

6.4.7 Verify all components of rotating fixture are secure and that VV is ready to rotate.

See Appendix A – Document Sign-off-Record

6.4.8 Using rotating crank handle and ratchet mechanism slowly rotate VV on its horizontal axis checking to see that CG is correct and not putting undue strain on the rotating mechanism.

Note: If VV CG is found to be off enough to cause rotating problem the support axle weldments will have to be moved or weight added to VV to shift the CG.

See Appendix A – Document Sign-off-Record

6.5 Metrology Set-up and Initial Vessel Measurements

6.5.1 Using a marker mark the positive toroidal field direction on the front and back surface of the vacuum vessel.

Note: The worm gear system is identified as the VV down direction. See Figure 5.

See Appendix A – Document Sign-off-Record

**Field Period Assembly Station One
D-NCSX-FPA-001**

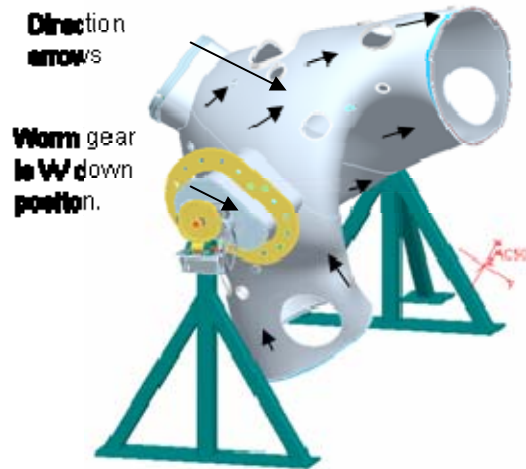


Figure 5 Arrows mark toroidal field direction

6.5.2 Rotate the VVSA through one full revolution and take note of the MTM supplied fiducial points. Determine whether the MTM supplied fiducials are adequate in number and location to allow alignment to the VVSA from any desired rotation on the turning fixture. Add additional fiducial points if required.

Note: Some monuments will be located on the body of the VVSA

6.5.3 Perform a best fit to the fiducial measurements using the monuments on the VV body. Settings will be made with the vessel NBI port at a $\pm 60^\circ$ off vertical position as indicated in Figure 6 and Figure 7. Secure vessel position by inserting release pin and tighten support axle cradle bolts. Verify that the mounting system is rigid enough to meet FP Dimensional Control Plan metrology requirements.

6.5.4 If additional fiducial points were added in step 6.5.2, measure their location.

See Appendix A – Document Sign-off-Record

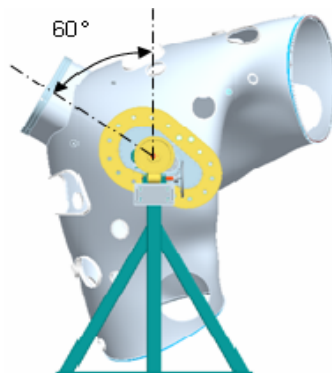


Figure 6 60° off vertical position

Field Period Assembly Station One D-NCSX-FPA-001

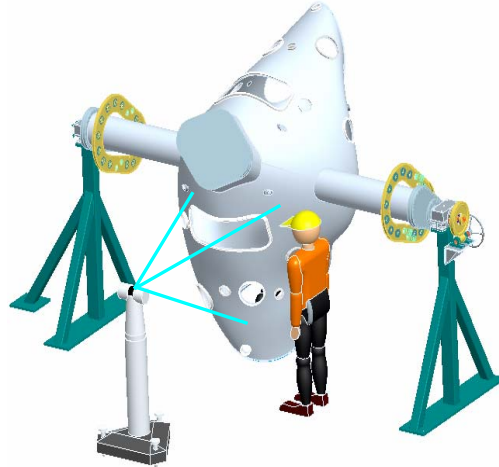


Figure 7 Vacuum Vessel in Rotated Position

6.6 Marking Flux Loop Template:

Each loop template has four locating notches which shall be used to install loops within $\pm 0.160''$ of marked locations, except for the loops at the symmetry points which shall be positioned within $\pm 0.020''$. Transfer the locator points for all copper templates to the measurement arm software. These points are the centers of the 0.020 inch radius semicircles machined on each side of a template. These are the ideal locations as defined in the CAD model. There will be some variation of the vessel surface from the CAD model and therefore the locator points. Installation will therefore be on a best fit basis recommended by the personnel responsible for the installation including metrology.

In general the templates are to be located within $.040''$ of the ideal, understanding that the vessel may vary radially to plus or minus 0.187 inch. One can define the tolerance as a point within a cylinder of $.040''$ radius and a radial extent of 0.375 inch.

The exceptions are the templates which define the Stellarator symmetry points. They're 15 such loops. These are to be located to a tolerance as a point within a cylinder of 0.25mm radius with a radial extent of 0.35 inches. The symmetry loops are located at theta 0 and 180 degrees, with poloidal centers on the NB ports and the period spacers. These loops are to be identically constructed and positioned on each of the 3 periods. These loops are templates 2-Th180-1 thru 2-Th-180-5.

When locating the templates, some of the fiducial points may be located such that they interfere with the template positioning. Individual fiducial points may be removed (and relocated if necessary), as long as there are sufficient additional fiducial points in the vicinity to allow for alignment and measurement of the relocated point

- 6.6.1 Secure vessel position with the 60° NBI port at a $\pm 60^\circ$ off vertical position by inserting release pin and tighten support axle cradle bolts.
- 6.6.2 Mark surface for 55 loop placements with the vessel NBI port at a $\pm 60^\circ$ off vertical position. It is expected that three metrology positions will be required on each side to accurately mark the vessel. The metrology system will be used to accurately define four marks (within $\pm 0.040''$) for each of the 55 loops except for the loops at the symmetry points which shall be positioned within $\pm 0.010''$. The magnetic loop locating points are to be permanently marked on the vessel surface. One method is to use a center punch. As each set of locator points are

Field Period Assembly Station One D-NCSX-FPA-001

marked, outline the rough geometry of the template, and circle the locator points. For ease of locating templates mark template number at center of four points. See figure 8 below and Reference drawing se 360-030-1a for loop designation, point marking details and model geometry data.

NOTE:

All Loop installation data to be logged on Table 1, 2 or 3 at end of procedure.

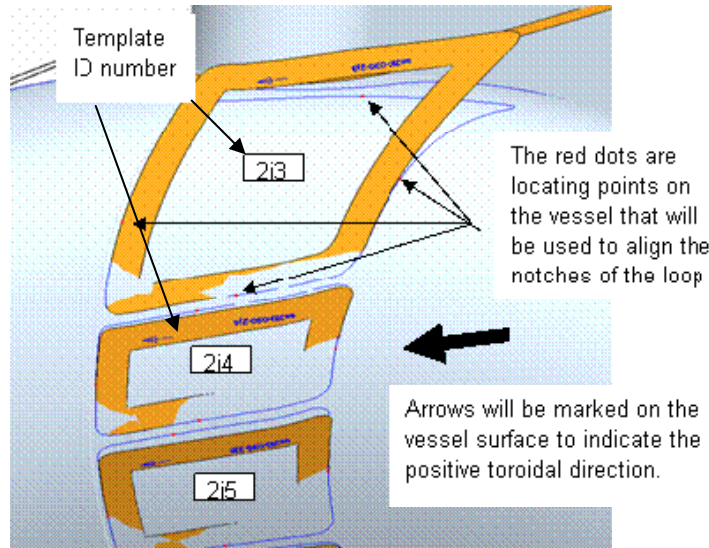


Figure 8 Template Locating and Numbering

6.7 Marking Heating Coolant Stud Locations:

6.7.1 The Leica or Roma Arm metrology system will be used to locate 356 studs per half period at X" spacing. Fine accuracy is not important position within +/- .50". The stud location shall be marked with a circle with a name designation added (A1, A2, A3....) to define the series. An outline of the coolant line and hold-down bracket shall also be marked. See Figure 9 and reference drawing se121-128 sheet 4 for cooling loop designation and locator point details.

Note: The cooling lines overlay the diagnostic loops.

All stud installation data to be logged on Table 3,4,or 5 at end of procedure.

Field Period Assembly Station One D-NCSX-FPA-001

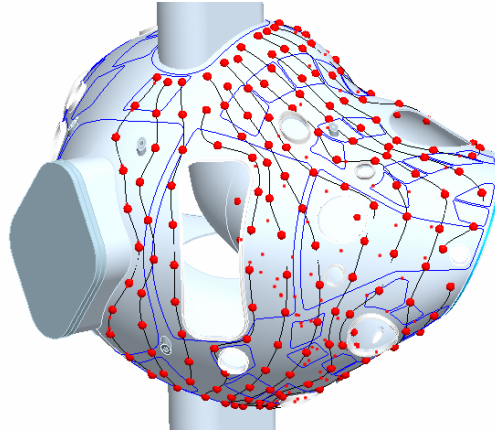


Figure 9 Overlays of the Coolant Lines over the Diagnostic Loops

6.8 Vertical Port Component Installation

- 6.8.1 Mark heating/cooling support bracket A and B attachment studs and mark bracket clip outline.
- 6.8.2 Install cryostat interface mounting flange on vertical ports. Before welding the interface flange on the vertical ports the cryostat interface flange must be moved into the proper assembly position. (See Figure 10).

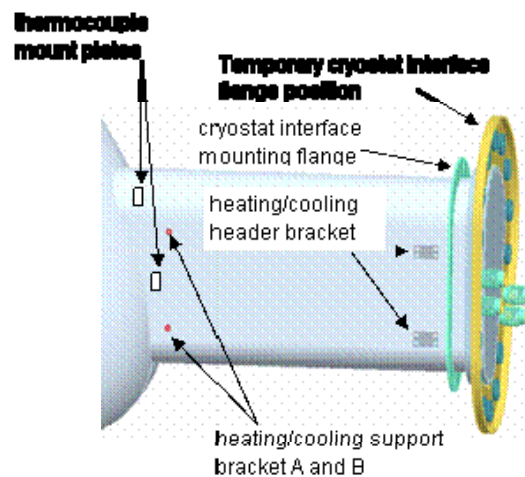


Figure 10 Cryostat Interface

- 6.8.3 Install cryostat interface flange on vertical ports.
- 6.8.4 Install heating/cooling header bracket.
- 6.8.5 Install thermocouple mounting plates and thermocouples to VV vertical ports. Reference drawing se 121-004.
- 6.8.6 Install heating strips on vessel vertical ports. See Figure 11.

**Field Period Assembly Station One
D-NCSX-FPA-001**

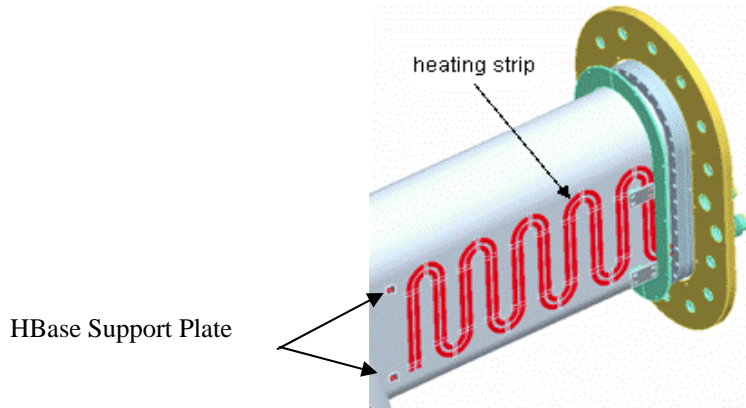


Figure 11 Heating strip

6.9 Installing of Magnetic Flux Loop Templates

- 6.9.1 Rotate VVSA to convenient installation position for locating loop templates. Each loop template has four locating notches which shall be used to install loops. Locate the template and fix it to the vessel using flat 316 SS shim stock clips (0.010 recommended, strong enough to hold the template yet developing a weak enough spot weld that can be easily removed with a chisel). Initially use only enough clips to support the template but allow it to be moved if need be. Using the metrology system verify the position of template and add additional clips securing the template at this position. If the tolerance deviation of the vessel does not allow the tolerance achievement of the loops then the cognizant physicist will determine the acceptable position. Installation will therefore be on a best fit basis to be approved by the physics and engineering cognizant and recommended by the personnel responsible for the installation including metrology. Symmetry Templates 2-Th180-1 thru 2-Th180-5 need to be placed and the flux loop wires run before adjacent loops are placed because of local template interferences. See Figure 8. After symmetry loop Templates 2-Th180-1 thru 2-T h180-5 are secured and positions verified, mark the path of the voltage loops on the vessel period surface. Proceed to step 6.10 and install flux loop wires for the five symmetry Loops.
- 6.9.2 Install all of the templates on the field period and log all information for each template on table 1 at end of procedure.

Note:

The locating direction arrow should be aligned in the general direction of the positive toroidal field direction arrows marked on the vessel surface. See Figure 12.

See Appendix A – Document Sign-off-Record

**Field Period Assembly Station One
D-NCSX-FPA-001**

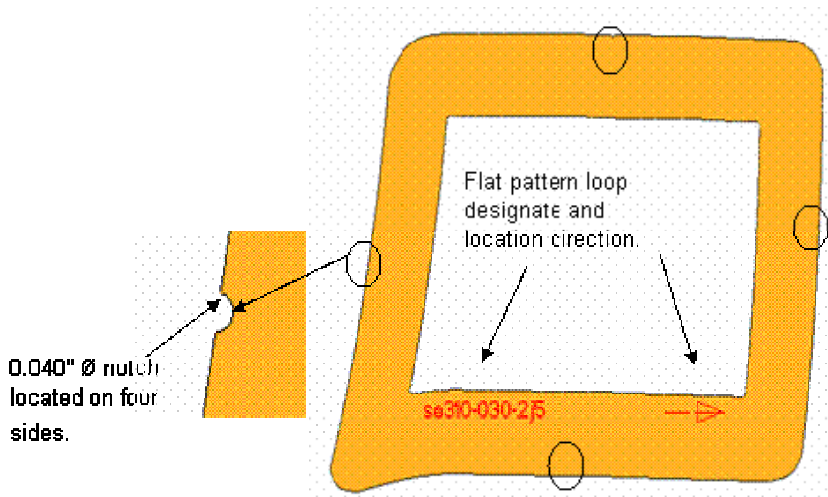


Figure 12 Installing Loop Templates

6.10 Installing of Magnetic Flux Loop

6.10.1 Each saddle Loop consists of a two turn coil of an inconel sheath and conductor, coaxial cable and twisted leads which run along the vessel surface and exit the cryostat region thru a 2.75 inch CF in the horse collar of a vertical port. The cables will be terminated in a junction box at a later time. Up to 20 twisted pairs will enter a JB.

Determine the unique length of co axial cable required for a complete loop including the twisted pair. Use a pliable yet non stretching material (stranded wire) to determine the circumference of the template and the developed length needed for the twisted pair along the marked path and along the vertical port and to the JB. If the circumference is designed as (C) and the twisted pair length as (L) then the total length (TL) required can be calculated as $TL=(2C+1) + 2(L+20) + (.667 \times L)$. This should result in about 20 inches of excess length at the JB box if the pitch is .625 inches and somewhat more if the pitch is closer to 0.75 inches. To determine L the starting point of the twisted pair must be determined.

At a few locations where the twisted pair cross a Voltage Loop the pitch will be interrupted and the pair will be run straight and parallel and touching for up to 2 inches. The voltage loop (single coaxial cable) will cross over the twisted pair at this location. This straight length pair will have a hold down clip on each side of the Voltage Loop and the Voltage Loop will have a hold down clip on either side of the twisted pair.

6.10.2 After the Loop length is determined cut the length from the large roll and remove all kinks and twists.

Seal both ends and the end on the large roll with the moisture barrier material provided. The MGO insulator is hygroscopic and must be sealed from moist air immediately after being cut.

½ inch wide by 3/8 inch deep indents have been provided along the edge of each template to accommodate the use of shim stock as hold downs. The hold downs are preformed and are 0.005 inch thick 316 SS. The clips are to have a magnetic permeability of less than 1.02. QA is to check a random sampling of 50 clips. High magnetic permeability can be mitigated by heat treating. There is sufficient space in an indent to accommodate 2 hold down clips. The partial clips are to be used to secure the inner turn and the full clips secure the outer turn. The copper

Field Period Assembly Station One D-NCSX-FPA-001

templates are 0.043 inch thick and have the central portion removed to facilitate conforming to the vessel surface and allow for the placement of the template holding clips. Use at least 4 spot welds to weld the clip to the vessel surface. Check each clip and ensure that the spot welds have punched through and the clip is secure.

- 6.10.3 The best point on the template to start the twisted pair was determined before the loop length was calculated therefore keeping this in mind start the wrap of the inner turn around the template and install a pre formed 0.005 inch thick SS partial clamp at each indent by spot welding, leaving sufficient space for the full clamp to be installed adjacent to it. In general the lower limit for the bend radius is $\frac{1}{4}$ inch. Minimize the dead space or excess area formed at the point where the inner and outer turns meet to start the twisted pair. Determine a method to form the same dead or excess area for all loops. This area will be added to the loop measurement area.
- 6.10.4 A simple plastic tool with two parallel holes drilled through has been developed to assist in the task of forming the twisted pairs. The twisted leads are to be identified with a 2 digit color band. There are less than 100 loops on the highest density field period. The twisted pair is to be identified in more than one location along its path and in the cryostat region, at least in the location under the horse collar and at the end of the cable inside the JB. The color bands must be retained at all times and when the excess length is cut and the termination made. All loop installation information and identifiers will be logged in Table 3 at end of procedure which will include loop tag nomenclature and color code number. The standard electrical wiring identifying convention will be used. Two different width bands will be used. The first number is the series will be the wider band with.
- The color identifiers are:
- | | |
|----------|----------|
| 0=Black | 5=Green |
| 1=Brown | 6=Blue |
| 2=Red | 7=Violet |
| 3=Orange | 8=Gray |
| 4=Yellow | 9=White |
- 6.10.5 After each twisted pair is installed it must be tested for continuity of the conductor and integrity of the MGO insulation. Log the test results for all pairs on Table 3. A dielectric fixture will be provided to facilitate the testing.
- 6.10.6 Install all remaining flux loop templates. Except for the mentioned wire runs in the previous step, all remaining templates shall be installed before any loop wires are run.
- 6.9.7 Mark vessel surface showing twisted pair leads path.

6.11 H/C stud and Loop wires installation.

NOTE:

1. **Use Reference drawing: se 123 008 and Dimensional Control Plan: NCSX-PLAN-FPA1DC-00.**
2. **Location of H/C tube mounting hardware in reference to Flux Loops must be considered before studs are welded on VVSA.**
3. **All H/C installation data to be logged on Table 7, 8, or 9 at end of procedure**

- 6.11.1 Install H/C studs on the VV being careful not to damage Flux Loops and Flux Loop Templates.

Field Period Assembly Station One D-NCSX-FPA-001

- 6.11.2 Install H/C tube hardware used for mounting H/C lines.
- 6.11.3 Install loop wires and then remove templates. Refer to drawing se 310-030-1a for guide in running voltage loops.
- 6.11.4 Use electrical color identifying code to mark wires as twisted wires leave template, along its path and after it passes through the horse collar.
- 6.11.5 Lay leads loosely to accommodate the installation of the H/C tube heat transfer bases.
- 6.11.6 Route excess lead length through the 2 ¾ Cryostat Flange and protect the excess length from damage.

6.12 Final Loop routing and Measurement

- 6.12.1 Perform final routing of flux leads and hold down with spot-welded shims stock straps spaced approximately 4" apart.

NOTE: The radial build of the twisted leads should not exceed 1/8", except in a few places (not under H/C tube paths) where it may be necessary for one set of leads to cross another.

- 6.12.2 Measure as-built paths of flux loops within ± 0.025 mm (0.010"). This shall be done by tracing the groove between the two turns of each loop using the Romer CMM arm with a small tip.

See Appendix A – Document Sign-off-Record

- 6.12.3 Using Reference drawing: se121-004 install thermocouple mount plates and thermocouples to VV shell.

6.13 Installation of H/C lines

- 6.13.1 Install H/C support bracket Weldment A and B and tube mount strap. See figure 13. and Reference Drawing: se121-00.

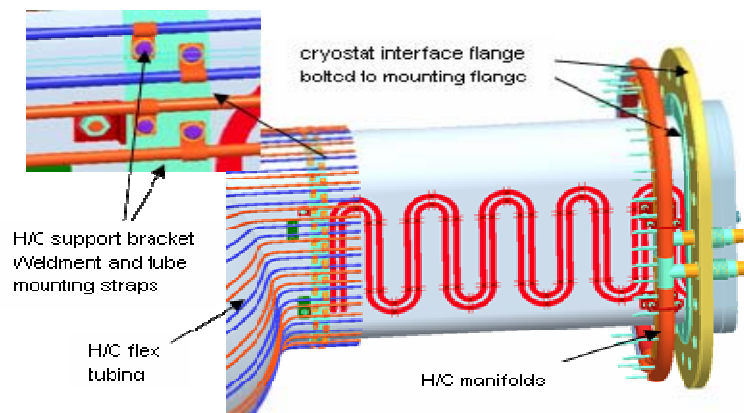


Figure 13 H/C Support Brackets

Field Period Assembly Station One D-NCSX-FPA-001

- 6.13.2 Using reference Drawings: sse121-008, se123-049 Install H/C cryostat flange and H/C manifolds. See Figure 13.
- 6.13.3 Using reference Drawings: sse121-008, se123-049 Install H/C flex tubing. See Figure 13.
- 6.13.4 Using reference Drawings: sse121-008, se123-049 Install H/C hard tubing. See Figure 14.

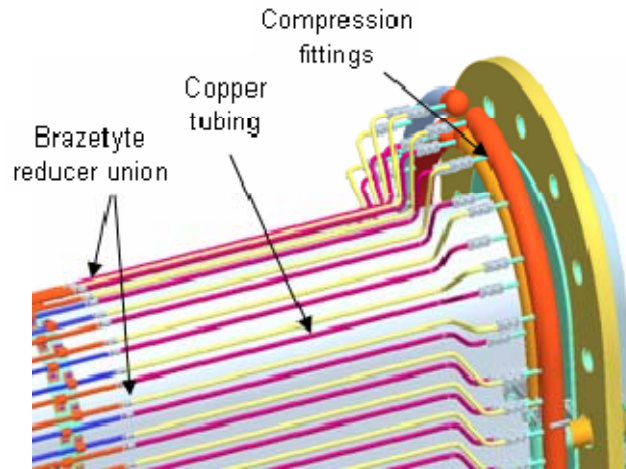


Figure 14 Hard Tube Installation

- 6.13.5 Leak check coolant lines.
Using engineering procedure ENG-014 (guidelines for Hydrostatic testing) test the individual cooling lines.
Note: Log leak check on table 7, 8, or 9.

See Appendix A – Document Sign-off-Record

6.14 Loop termination and verification check.

- 6.14.1 Perform final installation of twisted leads by checking continuity and resistance to ground of each pair. After H/C line bases are completed dress in cables and install hold down supports.
- 6.14.2 Verify tagging and conductors by physical check or use oscillator.
Note: Log continuity check and tagging on table 1,2,or 3.

See Appendix A – Document Sign-off-Record

- 6.14.3 Trim cable length – cut excess length to 1ft. using diamond wheel to cut end flat. This is accomplished by installing gas seal and partial junction box (JB); inserting CF gasket: routing cables thru predrilled holes in CF blank; routing cables thru pre-punched holes of silicon rubber gaskets; routing cables thru predrilled holes in JB base; installing CF threaded fasteners thru the JB base and torque to get metal contact between JB base and CF ring; and checking the cable configuration and condition in cryostat region.

**Field Period Assembly Station One
D-NCSX-FPA-001**

- 6.14.5 Terminate the cables by determining the length to terminal box (TB0; flat cut the cable with diamond wheel; strip back the sheath with tool provide leaving (TBD) of conductor exposed; cleaning the MGO from the conductor; apply a moisture barrier to MGO; and installing Teflon heat shrink tubing (4.1).
- 6.14.6 Strain relieve cables inside JB using spot welded SS shim stock.
- 6.14.7 Install TB circuit boards into front panel of JB and install conductors into TB.
- 6.14.8 Protect D sub connector by placing a protective cover over the D subminiature connector.
- 6.14.9 After the installation is complete, the as installed geometry and location of each saddle loop is to be measured and the data transferred to physics possibly through as intermediary since the data may be generated and stored as IGES files.

7. Completion of Activities at Station One:

7.1 Document Verification:

Verify that all pertinent data in the procedure tables 1, 2, 3, and Appendix A have been completed.

7.2 Field Package:

Ensure that all data sheets, photographs, QC inspection sheets, etc are included in the Field Package.

7.3 Approval:

Prior to releasing a VV from Station One it is required that the all-responsible individuals sign the release indicating that all processes at the station one have been satisfactorily completed. The release will include signatures from the Station Lead Technician, Field Supervisor and the QC representative.

All station one preparation activities including completion of appendix one and table 1,2,3, have been satisfactorily completed.

See Appendix A – Document Sign-off-Record

7.4 Preparing and Transferring Completed VV to Holding Area

- 7.4.1 Install the NB port temporary cover and NB angle support bracket. See Figure 16
- 7.4.2 Rotate VV to horizontal position. Secure in place by bolting down support axle cradle top support blocks and installing quick release pin.
- 7.4.3 Remove worm gear and install hoist rings.
- 7.4.4 Using lift procedure D-L-NCSX-997 remove completed VV from support stand and reposition to the vertical position with worm gear side of vessel in the down position.
- 7.4.5 While on the crane install base support plate. See Figure 15.

**Field Period Assembly Station One
D-NCSX-FPA-001**

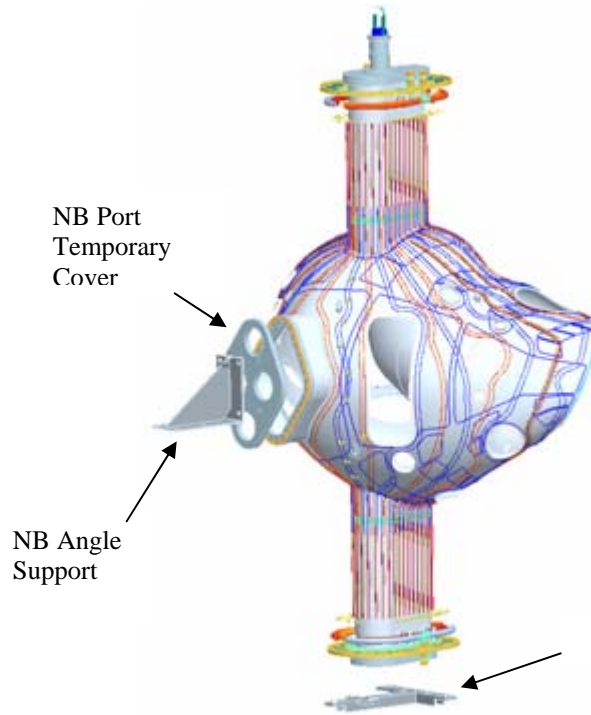


Figure 15 NB Angle Support Bracket and Base Support Plate

7.4.6 Position completed VV on Station 3 stand. See Figure 16.

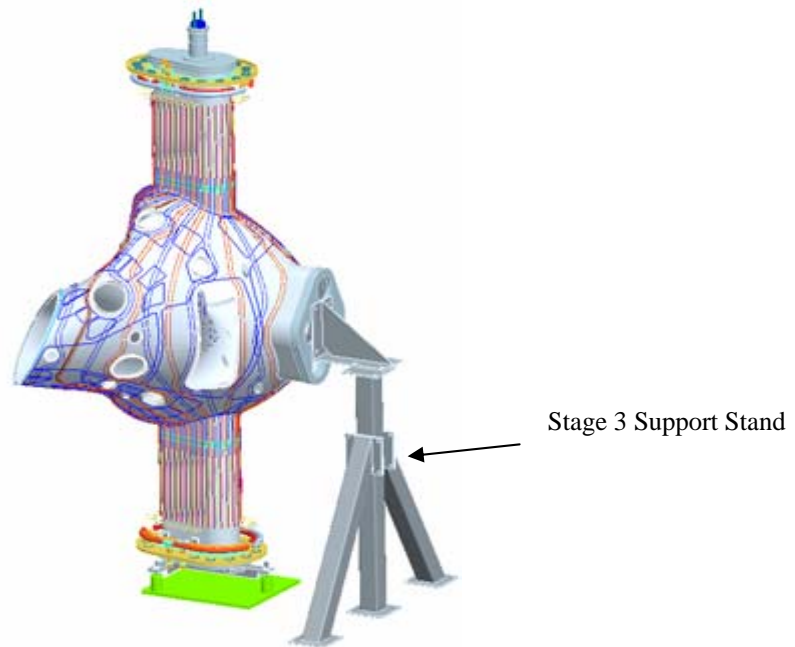


Figure 16 Stage 3 Support Stand

**Field Period Assembly Station One
D-NCSX-FPA-001**

8. Appendix A. Document Sign Off

1.3 Vacuum Vessel Segment Identification.

Segment Identification. _____ Verified by: _____ Date: _____ Lead Technician
--

4.1 Pre Job Briefing:

Pre Job Briefing Complete: _____ Date: _____ VV Field Supervisor Date
--

6.4.7 Rotating fixture secure:

Verified by: _____ Date: _____ Lead Technician
--

6.4.8 Cg verification:

Verified by: _____ Date: _____ Lead Technician
--

6.5.1 Arrows marked for toroidal field direction:

Verified by: _____ Date: _____ Lead Technician
--

6.5.4 Best fit to Fiducials :

Measurements taken by: _____ Date: _____
--

Measurements verified and /or approved by: _____ Date: _____ Metrology Engineer: _____ Date: _____

6.9.2 Loop Templates Best fit to Model:

Measurements taken by: _____ Date: _____
--

**Field Period Assembly Station One
D-NCSX-FPA-001**

Measurements verified and/or approved by:	
Metrology Engineer: _____	Date: _____

Physics Representative: _____	Date: _____

6.12.2 Final Loop Measurements:

Measurements taken by: _____	Date: _____
-------------------------------------	--------------------

Measurements verified and/or approved by:	
Metrology Engineer: _____	Date: _____
Physics Representative: _____	Date: _____

6.13.5 Leak Check Coolant Lines:

Verified by: _____	Date: _____
Lead Technician	
QC Representative: _____	Date: _____

6.14.2 Loop Termination Continuity Check:

Verified by: _____	Date: _____
Lead Technician	
QC Representative: _____	Date: _____

**Field Period Assembly Station One
D-NCSX-FPA-001**

7.3 Approval:

All station one preparation activities including completion of appendix one and table 1,2,3, have been satisfactorily completed.

QC shall verify completion of documentation:

Quality Control Representative: _____ Date: _____

The VV is ready for transfer to the VV station no. 3:

Lead Technician: _____ Date: _____
Field Supervisor: _____ Date: _____
Quality Control Representative: _____ Date: _____

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 1-Loop Installation Data For Field Period 1

Loop	Metrology	Initial	Template	Template	Loops	Loop	Loop	Continuity	Tagging	Comments
I.D.	Position	Points Located	Placed	Verified	Placed	Measured Length	Length Verified	Checked	Verified	
AA1										
CC3										
CC5										
D1										
D3										
D7										
E1										
F4										
F6										
F10										
FF2										
FF4										
FF5										
G7										
GG1										
GG3										
GG5										
GG9										
GG11										
H4										
H8										
HH6										
HH10										
I7										
J9										

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 1-Loop Installation Data For Field Period 1

Loop	Metrology	Initial	Template	Template	Loops	Loop	Loop	Continuity	Tagging	Comments
I.D.	Position	Points Located	Placed	Verified	Placed	Measured Length	Length Verified	Checked	Verified	
JJ5										
K2										
K4										
K7										
K11										
KK3										
KK8										
KK9										
L6										
L9										
LL5										
M2										
M9										
MM1										
MM10										
N2										
N5										
N6										
N9										
NN1										
NN4										
NN8										
NN11										
O6										
OO5										

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 2-Loop Installation Data For Field Period 2

Loop	Metrology	Initial	Template	Template	Loops	Loop	Loop	Continuity	Tagging	Comments
I.D.	Position	Points Located	Placed	Verified	Placed	Measured Length	Length Verified	Checked	Verified	
AA2										
B2										
C1										
CC4										
D4										
D5										
D7										
DD2										
DD5										
E2										
EE7										
F8										
F11										
FF3										
FF7										
G1										
G4										
G8										
GG10										
H4										
HH2										
HH5										
HH7										
HH10										
I4										

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 2-Loop Installation Data For Field Period 2

Loop	Metrology	Initial	Template	Template	Loops	Loop	Loop	Continuity	Tagging	Comments
I.D.	Position	Points Located	Placed	Verified	Placed	Measured Length	Length Verified	Checked	Verified	
II1										
II2										
II3										
II4										
II5										
II6										
II7										
II8										
II9										
J1										
J2										
J3										
J4										
J5										
J6										
J7										
J8										
J9										
J10										
JJ2										
K5										
K9										
L1										
L3										
LL2										

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 2-Loop Installation Data For Field Period 2

Loop	Metrology	Initial	Template	Template	Loops	Loop	Loop	Continuity	Tagging	Comments
I.D.	Position	Points Located	Placed	Verified	Placed	Measured Length	Length Verified	Checked	Verified	
LL4										
LL7										
M4										
MM5										
N2										
N7										
NN1										
NN3										
O7										
O10										
OO8										
PP4										
THO-1										
THO-2										
THO-3										
THO-4										
THO-5										
THO180-1										
THO180-2										

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 3-Loop Installation Data For Field Period 3

Loop	Metrology	Initial	Template	Template	Loops	Loop	Loop	Continuity	Tagging	Comments
I.D.	Position	Points Located	Placed	Verified	Placed	Measured Length	Length Verified	Checked	Verified	
B1										
B4										
BB3										
CC2										
D6										
DD3										
DD4										
E3										
E4										
E5										
EE6										
F9										
FF1										
FF9										
G2										
G8										
GG6										
H1										
H3										
H11										
HH7										
HH9										
I2										
I8										
JJ4										

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 3-Loop Installation Data For Field Period 3

Loop	Metrology	Initial	Template	Template	Loops	Loop	Loop	Continuity	Tagging	Comments
I.D.	Position	Points Located	Placed	Verified	Placed	Measured Length	Length Verified	Checked	Verified	
JJ8										
K6										
KK1										
KK7										
KK8										
KK10										
L2										
L8										
LL8										
LL10										
M3										
M7										
M8										
MM6										
MM8										
MM11										
N10										
O11										
O4										
O9										
O11										
OO2										
OO3										
OO4										
OO7										

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 3-Loop Installation Data For Field Period 3

Loop	Metrology	Initial	Template	Template	Loops	Loop	Loop	Continuity	Tagging	Comments
I.D.	Position	Points Located	Placed	Verified	Placed	Measured Length	Length Verified	Checked	Verified	
OO10										
PP1										
Q2										
QQ1										
THO-1										
THO-2										
THO-3										
THO-4										
THO-5										
TH180-1										
TH180-2										
TH180-3										
TH180-4										
TH180-5										

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 4-Stud Installation Data for Field Period 1:

TBD

Field Period Assembly Station One
D-NCSX-FPA-001

Table 5-Stud Installation Data for Field Period 2:

TBD

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 6-Stud Installation Data for Field Period 3:

TBD

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 7-H/C/ Lines Installation and Leak Check Data Field Period 1:

TBD

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 8-H/C/ Lines Installation and Leak Check Data Field Period 2:

TBD

**Field Period Assembly Station One
D-NCSX-FPA-001**

Table 9-H/C/ Lines Installation and Leak Check Data Field Period 3:

TBD